

Microleakage and mechanical behavior of conical vs. internal hexagon implant-abutment prosthetic connection under a cyclic load fatigue test

F. LORUSSO¹, A. GRECO LUCCHINA¹, F. ROMANO¹, G. FALISI²,
M.S. DI CARMINE³, C. BUGEA⁴, A. SCARANO^{4,5}

¹Department of Innovative Technologies in Medicine and Dentistry, University of Chieti-Pescara, Chieti-Pescara, Italy

²Department of Life Health and Environmental Sciences, University of L'Aquila, L'Aquila, Italy

³Interdisciplinary Department of Medicine, "Aldo Moro" University of Bari, Bari, Italy

⁴Department of Innovative Technologies in Medicine and Dentistry, University of Chieti-Pescara, Chieti-Pescara, Italy

⁵Department of Oral Implantology, Dental Research Division, College Ingà, UNINGÁ, Cachoeiro de Itapemirim, Espírito Santo, Brazil

G. Falisi and A. Greco Lucchina contributed equally to this work as co-first Authors

M.S. Di Carmine and C. Bugea contributed equally to this work as co-last Authors

Abstract. – OBJECTIVE: The aim of the present investigation was to evaluate, by an in vitro simulation, the mechanical behavior of the conical regular, conical narrow and internal hexagon under cyclic load and the microleakage of the prosthetic connection of the fixture.

MATERIALS AND METHODS: A standardized cyclic loading was performed for the implant with conical connection (diameter 4 mm - length 10 mm) (CS) and internal hexagon connection (diameter 4 mm - length 10 mm) (IH). The toluidine blue infiltration was evaluated with the paper cone test.

RESULTS: After a total of 5×10^4 loads, the screw was removed, and the abutment appear solid and stable to the implant fixture for CS, while the IH was unstable. There was no infiltration of the toluidine marker in the connection interfaces of CS implants, while the IH was positive to the paper cone test.

CONCLUSIONS: The study data showed that the conical connection showed higher stability compared to the internal hexagon connection under the loading and it is able to prevent bacterial microleakage. This effectiveness should be considered for the long-term maintenance of the peri-implant soft and hard tissues around the fixture.

Key Words:

Implant/abutment, Micro gap, Crestal bone remodeling, Conical connection, Cyclic loading.

Introduction

Dental implants are medical devices, biocompatible and surgical inserted into the jawbone, mainly for prosthetic purposes, to replace one or more missing teeth¹⁻⁴. Nowadays, the implant supported prostheses are extremely predictable. The success rate of dental implants, as shown by Papaspyridakos et al⁵, exceeds 90% abundantly with 5 years follow-ups. However, crestal bone loss has been observed for decades around successfully integrated dental implants. Bone loss is significant in the first year while in the following years decreases dramatically^{6,7}, Adell et al⁸ were the first to report and quantify a marginal bone loss that was around 1.5 mm in the first year with variability between 0 and 3 mm. In the following years, the bone loss was around 0.05 and 0.13⁸. This study about the causes of bone loss is fundamental because bone loss may influence aesthetic outcomes and can interfere with the long-term health of the peri-implant tissues and with the long-term prognosis of the implant⁹⁻¹². The vast majority of implants consist of a fixture and an abutment that are coupled through connections¹³⁻¹⁶. However, a virtual micro gap space is produced at the level of the interface between the implant components. This

which seems to be responsible for a peri-implant inflammatory infiltrate, a consequence of the fact that bacteria can proliferate precisely between the abutment and the fixture^{6,9,17,18}. The majority of dental implants are composed by an abutment and a fixture coupled with connections screwed^{19,20-23}. The micro gap can also lead to an altered distribution of the masticatory stresses with the danger of unscrewing and breakage for the components, and consequently it could produce a peri-implant bone resorption¹⁹.

The bacterial infiltration between the implant and the abutment is called microleakage. It has been found to occur in static conditions and seems to increase when the assemblies are loaded²³. Loading forces on the prosthetic restoration under function may cause bending of the components or movements inside the implant system, with the formation of a larger gap, determining a “pump” effect that probably increases the movement of the microorganisms^{6,23}. The aim of this study is to evaluate *in vitro* two different types of implants connection under cyclic load and the possible microleakage of the prosthetic connection of the fixture.

Materials and Methods

For this *in vitro* study a total of 8 implants were used: 15 Sirio implants 4 mm ×10 mm with a screw-retained internal hexagon (IH) and 15 Close BL implants 4 mm × 10 mm with a screw-retained conical abutment connection (CS); (Isomed, Due Carrare, Italy). All the samples were subjected to a cyclic load 5×10^4 times. The load was applied on a cap placed on the abutment. Implants and abutments were screwed at 30 N/cm as indicated by the manufacturer. To hold the implant into the desired position, a hole in a resin block was performed. The implants were inserted into the resin block with a 30° inclination to simulate masticatory forces. The implant-abutment connection was left out for about 3 mm from the resin block to simulate the worst bone condition. The resin blocks were designed by a 3D builder software (Microsoft, Redmond WA, USA) and the master model was printed by 3D resin printer (New Kinpo Group, New Taipei City, Taiwan). After that, the master model was used to realize all the resin blocks to reproduce all the experimental conditions required. All samples were loaded with a universal test machine Lloyd 30k (Lloyd Instrument Ltd,

Segensworth, UK) managed by the Nxygen 4.0 software (Ametek, Berwyn, Pennsylvania, USA), to reproduce a load between 20 N/cm and 300 N/cm with a frequency of 4 Hz²³. 0.7 µL of toluidine blue were placed into a cylinder on the resin block. At the end of the cyclic loads, the toluidine blue was eliminated, and the possible marker infiltration was evaluated by the “point test” with a paper cone put at the implant-abutment connection after the unscrewing of components. The possible toluidine blue on the paper cone was then misused.

Statistical Analysis

The power analysis has been conducted accordingly to the findings of a previous study²⁴. The sample size calculation has been conducted by the Fisher's exact test [a err: 0.05; Power (1-b): 80%; p1: 0.6; p2: 0.1; allocation ratio: 1:1]. The minimum statistical sample size was 13 specimens for each experimental condition that was augmented to 15 samples for each study group as compensation for eventual test drop-out. The study data were collected in a specially designed electronic database and analyzed by the statistical software package GraphPad 9 (La Jolla, CA, USA). The study data were analyzed by the Chi-square test and a $p < 0.05$ was considered the reference for the statistical significance.

Results

Group CS (Conical Connection)

After one week and about 5×10^4 loads, 15 samples with standard conical connections were unscrewed. All samples of this group had a stable abutment at the fixture. No marker of toluidine blue was found at the implant-abutment interface. The paper point test was negative (Figures 1-2) (Table I-II).

Group IH (Internal Hexagon)

After one week and about 5×10^4 loads, 15 samples with internal hexagon connection were unscrewed and 5 sample was stable. All abutments of this group were unstable due to the loosening of the fixing screw. The marker toluidine blue was visible at the implant-abutment interface and the paper point test was positive (Figure 3-5) (Table I-II).



Figure 1. Preparation of the CS and IH implants specimens for the experimental tests. Both groups after submitted to 5×10^4 loads to evaluate the microlleakage through toluidine blue infiltration.

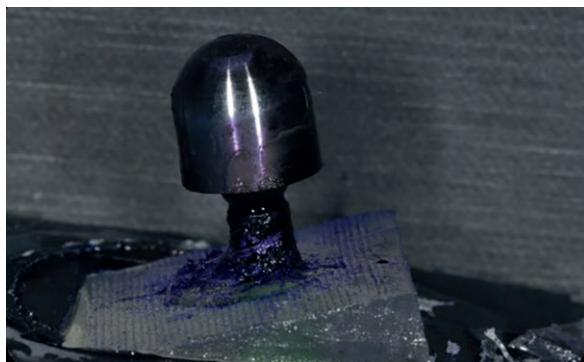


Figure 2. Specimen at the end of the loading test.

Discussion

Many authors^{6,17,20,23} have studied the space at the implant-abutment junction. The problem

of the micro gap is biological and mechanical. The biological problem relates to the presence of bacteria that, *in vivo*, can produce a bacterial reservoir that, in turn, interferes with the long-term health of the peri-implant tissues and with the long-term prognosis of the implant^{10,25-33}. The mechanical problem relates to micromovement and possible loosening or fracturing of screw-retained abutments^{17,34}. The precise mechanism responsible for the crestal bone remodeling in 2-piece implants is not known^{11,34-39}. The existence of a bacterial leakage, both at the junction between the abutment and the implant, and along the abutment screw has been reported²³. This crestal bone resorption has not been observed around sleeping implants, where both exposures to microbial colonization and loading were absent⁴⁰. It has been shown that inflam-

Table I. Summary of the linear deformation (mm), average loading (N), minimum loading (N) and maximum loading (N) of the CS and IH implants

Implant tested	Linear deformation (mm)	Average loading (N)	Minimum loading (N)	Maximum loading (N)
CS	0.609157991 ± 0.28	$200 \text{ N} \pm 13.5$	186.67 ± 10.2	216.86 ± 12.7
IH	0.887846462 ± 0.30	$200 \text{ N} \pm 14.4$	189.08 ± 11.3	213.17 ± 12.2
<i>p</i> -value	$p > 0.05$	$p > 0.05$	$p > 0.05$	$p > 0.05$

No significant difference was detected between the two groups after 5×10^4 loads ($p > 0.05$, Student *t*-test).

Table II. Summary of the Chi-square test of the study groups comparison.

Contingency: prospective data	
Test	Chi-square
Chi-square, df	6.000, 1
Z	2.449
p-value	0.0143
p-value summary	*
One- or two-sided?	Two-sided
Statistically significant ($p < 0.05$)?	Yes

* $p < 0.05$.

mation occurs if the abutment loosens on the implants placed in a submerged approach, with a possible fistula formation^{41,42}. There is a physiological reaction to the presence of an interface; the reason for this reaction is unknown, but it may be related to bacterial contamination or micromovements of the interface^{43,44}. Due to these problems, the manufacturers have proposed different implant-abutment connection designs to

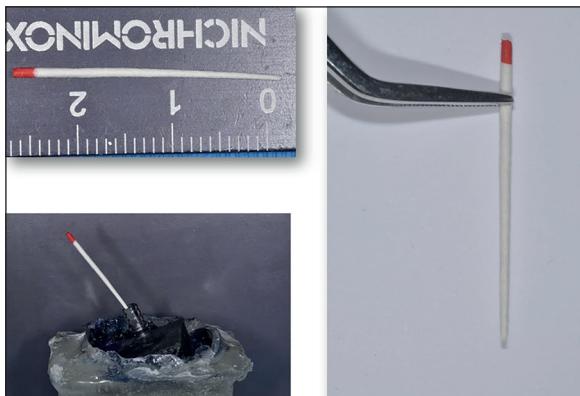


Figure 3. Toluidine blue infiltration measured by a paper cone. CS implant showed no marginal infiltration after the loading test.

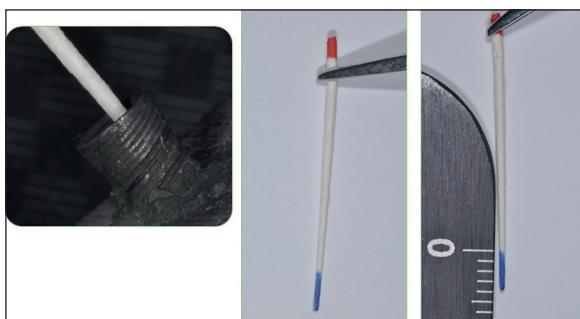


Figure 4. Positivity to toluidine blue infiltration measured by a paper cone (IH group).

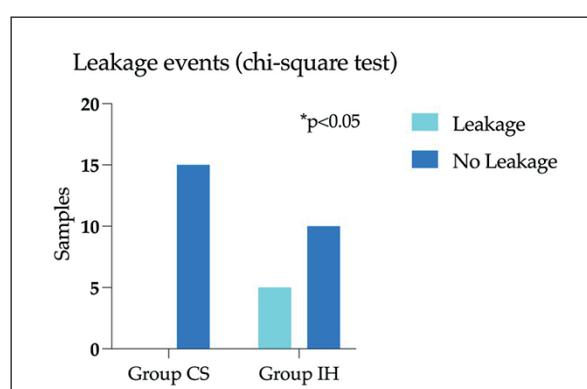


Figure 5. Chart of the leakage events associated to the study groups comparison after 5×10^4 times cycles.

achieve a better reliability and better seal between the components^{24,45}. In the present *in vitro* study, we have compared the internal hexagon connection (IH) and conical connection (CS). The samples were evaluated after cyclic loads to reproduce the masticatory loads inside the oral cavity. The effectiveness shows how the internal hexagon connections are less reliable in preventing microleakage, because in each sample of this group, the abutment screw was loosened, and toluidine blue was found inside the connection. Both conical connections, standard and narrow, have not shown a screw loosening, and no toluidine blue infiltration inside the implant-abutment junction with a negative paper point.

Conclusions

In this *in vitro* study, both conical connections, standard and narrow diameter, seem more reliable than the internal hexagon in preventing bacterial microleakage and obtaining a more stable implant-abutment connection. These sealing capacities suggest that conical connection should be used, especially for the treatment of clinical cases with high aesthetic and functional value, where long-term stability of the peri-implant tissues is required.

Conflict of Interest

The Authors declare that they have no conflict of interests.

Funding

This study did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

Availability of Data and Materials

All data generated or analyzed during this study are included in this published article.

Authors' Contribution

All authors were involved in the literature review and performance of the investigation. All authors read and approved the final manuscript.

Ethics Approval

Not applicable..

Informed Consent

Not applicable..

ORCID ID

Felice Lorusso: 0000-0002-2660-9231; Alberta Greco Lucchina: 0000-0002-1985-4263; Francesco Romano: 0000-0002-8005-2817; Giovanni Falisi: 0000-0001-5166-9861; Calogero Bugea: 0000-0002-9960-9830; Maria Stella Di Carmine: 0000-0003-4849-9982; Antonio Scarano: 0000-0003-1374-6146.

References

- 1) Davies JE. Understanding peri-implant endosseous healing. *J Dent Educ* 2003; 67: 932-949.
- 2) Albrektsson T, Berglundh T, Lindhe J. Osseointegration: Historic background and current concepts. *Clin Perio Impl Dent* 2003; 4: 809-820.
- 3) Albrektsson T, Wennerberg A. On osseointegration in relation to implant surfaces. *Clin Implant Dent Relat Res* 2019; 21: 4-7.
- 4) Albrektsson T, Sennerby L. State of the art in oral implants. *J Clin Periodontol* 1991; 18: 474-481.
- 5) Papaspyridakos P, Chen CJ, Singh M, Weber HP, Gallucci GO. Success criteria in implant dentistry: a systematic review. *J Dent Res* 2012; 91: 242-248.
- 6) Zandim-Barcelos DL, Carvalho GG de, Sapata VM, Villar CC, Hämmmerle C, Romito GA. Implant-based factor as possible risk for peri-implantitis. *Braz Oral Res* 2019; 33: 67.
- 7) Scarano A, Piattelli A, Polimeni A, Di Iorio D, Carinci F. Bacterial adhesion on commercially pure titanium and anatase-coated titanium healing screws: an in vivo human study. *J Periodontol* 2010; 81: 1466-1471.
- 8) Adell R, Lekholm U, Rockler B, Bränemark PI. A 15-year study of osseointegrated implants in the treatment of the edentulous jaw. *Int J Oral Surg* 1981; 10: 387-416.
- 9) Shemtov-Yona K, Rittel D, Levin L, Machtei EE. Effect of dental implant diameter on fatigue performance. Part I: mechanical behavior. *Clin Implant Dent Relat Res* 2014; 16: 172-177.
- 10) Tumedei M, Piattelli A, Degidi M, Mangano C, Iezzi G. A Narrative Review of the Histological and Histomorphometrical Evaluation of the Peri-Implant Bone in Loaded and Unloaded Dental Implants. A 30-Year Experience (1988-2018). *Int J Environ Res Public Health* 2020; 17: 2088.
- 11) On SW, Yi SM, Park IY, Byun SH, Yang BE. Fracture and Fatigue of Dental Implants Fixtures and Abutments with a Novel Internal Connection Design: An In Vitro Pilot Study Comparing Three Different Dental Implant Systems. *J Funct Biomater* 2022; 13: 239.
- 12) Brożek R, Koczorowski R, Dorocka-Bobkowska B. Laboratory and clinical evaluation of polymer materials reinforced by fibers used in dentistry. *Eur Rev Med Pharmacol Sci* 2019; 23: 1855-1863.
- 13) Comuzzi L, Tumedei M, Piattelli A, Iezzi G. Short vs. Standard Length Cone Morse Connection Implants: An In Vitro Pilot Study in Low Density Polyurethane Foam. *Symmetry* 2019; 11: 1349.
- 14) Comuzzi L, Tumedei M, Pontes AE, Piattelli A, Iezzi G. Primary Stability of Dental Implants in Low-Density (10 and 20 pcf) Polyurethane Foam Blocks: Conical vs Cylindrical Implants. *Int J Environ Res Public Health* 2020; 17: 2617.
- 15) Tumedei M, Piattelli A, Falco A, De Angelis F, Lorusso F, Di Carmine M, Iezzi G. An in vitro evaluation on polyurethane foam sheets of the insertion torque, removal torque values, and resonance frequency analysis (RFA) of a self-tapping threads and round apex implant. *Cell Polymers* 2020; 1: 1796.
- 16) Kim KS, Lim YJ. Axial Displacements and Removal Torque Changes of Five Different Implant-Abutment Connections under Static Vertical Loading. *Materials* 2020; 13: 699.
- 17) Assenza B, Scarano A, Leghissa G, Carusi G, Thams U, Roman FS, Piattelli A. Screw- vs cement-implant-retained restorations: an experimental study in the Beagle. Part 1. Screw and abutment loosening. *J Oral Impl* 2005; 31: 242-246.
- 18) Cumbo C, Marigo L, Somma F, La Torre G, Minniciacchi I, D'Addona A. Implant platform switching concept: a literature review. *Eur Rev Med Pharmacol Sci* 2013; 17: 392-397.
- 19) Nissan J, Narobai D, Gross O, Ghelfan O, Chaushu G. Long-term outcome of cemented versus screw-retained implant-supported partial restorations. *Int J Oral Maxillofac Implants* 2011; 26: 1102-1107.
- 20) Lepesqueur LS, de Figueiredo VMG, Ferreira LL, Sobrinho AS da S, Massi M, Bottino MA, Nogueira Junior L. Coating dental implant abutment screws with diamondlike carbon doped with diamond nanoparticles: the effect on maintaining torque after mechanical cycling. *Int J Oral Maxillofac Implants* 2015; 30: 1310-1316.
- 21) Scarano A, Assenza B, Piattelli M, Iezzi G, Leghissa GC, Quaranta A, Tortora P, Piattelli A. A 16-year study of the microgap between 272 human titanium implants and their abutments. *J Oral Implantol* 2005; 31: 269-275.

22) Scarano A, Mortellaro C, Mavriqi L, Pecci R, Valbonetti L. Evaluation of Microgap With Three-Dimensional X-Ray Microtomography: Internal Hexagon Versus Cone Morse. *J Craniofac Surg* 2016; 27: 682-285.

23) Assenza B, Tripodi D, Scarano A, Perrotti V, Piattelli A, Iezzi G, D'Ercole S. Bacterial leakage in implants with different implant-abutment connections: an in vitro study. *Journal of Periodontology* 2012; 83: 491-497.

24) Scarano A, Perrotti V, Piattelli A, Iaculli F, Iezzi G. Sealing capability of implant-abutment junction under cyclic loading: a toluidine blue in vitro study. *J Appl Biomater Funct Mater* 2015; 13: 293-295.

25) Vinhas AS, Aroso C, Salazar F, López-Jarana P, Ríos-Santos JV, Herrero-Climent M. Review of the Mechanical Behavior of Different Implant-Abutment Connections. *Int J Environ Res Public Health* 2020; 17: 8685.

26) Fujiwara S, Kato S, Bengazi F, Urbizo Velez J, Tumedei M, Kotsu M, Botticelli D. Healing at implants installed in osteotomies prepared either with a piezoelectric device or drills: an experimental study in dogs. *Oral Maxillofac Surg* 2020; 25: 65-73.

27) Kotsu M, Urbizo Velez J, Bengazi F, Tumedei M, Fujiwara S, Kato S, et al. Healing at implants installed from ~ 70- to < 10-Ncm insertion torques: an experimental study in dogs. *Oral Maxillofac Surg* 2020; 25: 55-64.

28) Kim KS, Lim YJ. Axial Displacements and Removal Torque Changes of Five Different Implant-Abutment Connections under Static Vertical Loading. *Materials* 2020; 13: 699.

29) Basgil MC, Kurtoglu C, Soygun K, Uslan Y, Demi RT. Dynamic and static load performance of dental biomaterial systems with conical implant-abutment connections. *Biomed Mater Eng* 2020; 31: 319-328.

30) Borges FL, Dias RO, Piattelli A, Onuma T, Gouveia Cardoso LA, Salomão M, Scarano A, Ayub E, Shibli JA. Simultaneous sinus membrane elevation and dental implant placement without bone graft: a 6-month follow-up study. *J Periodontol* 2011; 82: 403-12.

31) Sun F, Lv LT, Cheng W, Zhang JL, Ba DC, Song GQ, Lin Z. Effect of Loading Angles and Implant Lengths on the Static and Fatigue Fractures of Dental Implants. *Materials* 2021; 14: 5542.

32) Park SJ, Lee SW, Leesungbok R, Ahn SJ. Influence of the connection design and titanium grades of the implant complex on resistance under static loading. *J Adv Prosthodont* 2016; 8: 388-395.

33) Maglione M, Bevilacqua L, Dotto F, Costantinides F, Lorusso F, Scarano A. Observational Study on the Preparation of the Implant Site with Piezosurgery vs. Drill: Comparison between the Two Methods in terms of Postoperative Pain, Surgical Times, and Operational Advantages. *BioMed Res Int* 2019; 1: 8483658.

34) Scarano A, Carinci F, Lorusso F, Festa F, Bevilacqua L, Santos de Oliveira P, Maglione M. Ultrasonic vs Drill Implant Site Preparation: Post-Operative Pain Measurement Through VAS, Swelling and Crestal Bone Remodeling: A Randomized Clinical Study. *Materials* 2018; 11: 1.

35) Geramizadeh M, Katoozian H, Amid R, Kadkhodazadeh M. Static, Dynamic, and Fatigue Finite Element Analysis of Dental Implants with Different Thread Designs. *J Long Term Eff Med Implants* 2016; 26: 347-355.

36) Assenza B, Scarano A, Petrone G, Iezzi G, Thams U, San Roman F, Piattelli A. Crestal bone remodeling in loaded and unloaded implants and the microgap: a histologic study. *Imp Dent* 2003; 12: 235-241.

37) Anitua E, Murias-Freijo A, Alkhraisat MH. Implant Site Under-Preparation to Compensate the Remodeling of an Autologous Bone Block Graft. *J Craniofac Surg* 2015; 26: 374-377.

38) Gehrke SA, Júnior JA, Treichel TLE, do Prado TD, Dedavid BA, de Aza PN. Effects of insertion torque values on the marginal bone loss of dental implants installed in sheep mandibles. *Sci Rep* 2022; 12: 538.

39) Noumbissi S, Scarano A, Gupta S. A Literature Review Study on Atomic Ions Dissolution of Titanium and Its Alloys in Implant Dentistry. *Materials* 2019; 12: 368.

40) Smeets R, Henningsen A, Jung O, Heiland M, Hammächer C, Stein JM. Definition, etiology, prevention and treatment of peri-implantitis--a review. *Head Face Med* 2014; 3: 10-34.

41) Agustín-Panadero R, Serra-Pastor B, Roig-Vanaclocha A, Fons-Font A, Solá-Ruiz MF. Fracture resistance and the mode of failure produced in metal-free crowns cemented onto zirconia abutments in dental implants. *PLoS One* 2019; 14: 0220551.

42) Mishra SK, Chowdhary R, Kumari S. Microleakage at the Different Implant Abutment Interface: A Systematic Review. *J Clin Diagn Res* 2017; 11: 10-15.

43) Atsuta I, Ayukawa Y, Kondo R, Oshiro W, Matsuura Y, Furuhashi A, Tsukiyama Y, Koyano K. Soft tissue sealing around dental implants based on histological interpretation. *J Prosthodont Res* 2016; 60: 3-11.

44) Etter TH, Häkanson I, Lang NP, Trejo PM, Caffesse RG. Healing after standardized clinical probing of the perimplant soft tissue seal: a histomorphometric study in dogs. *Clin Oral Implants Res* 2002; 13: 571-580.

45) Scarano A, Lorusso C, Di Giulio C, Mazzatorta A. Evaluation of the Sealing Capability of the Implant Healing Screw by Using Real Time Volatile Organic Compounds Analysis: Internal Hexagon Versus Cone Morse. *J Periodontol* 2016; 87: 1492-1498.